
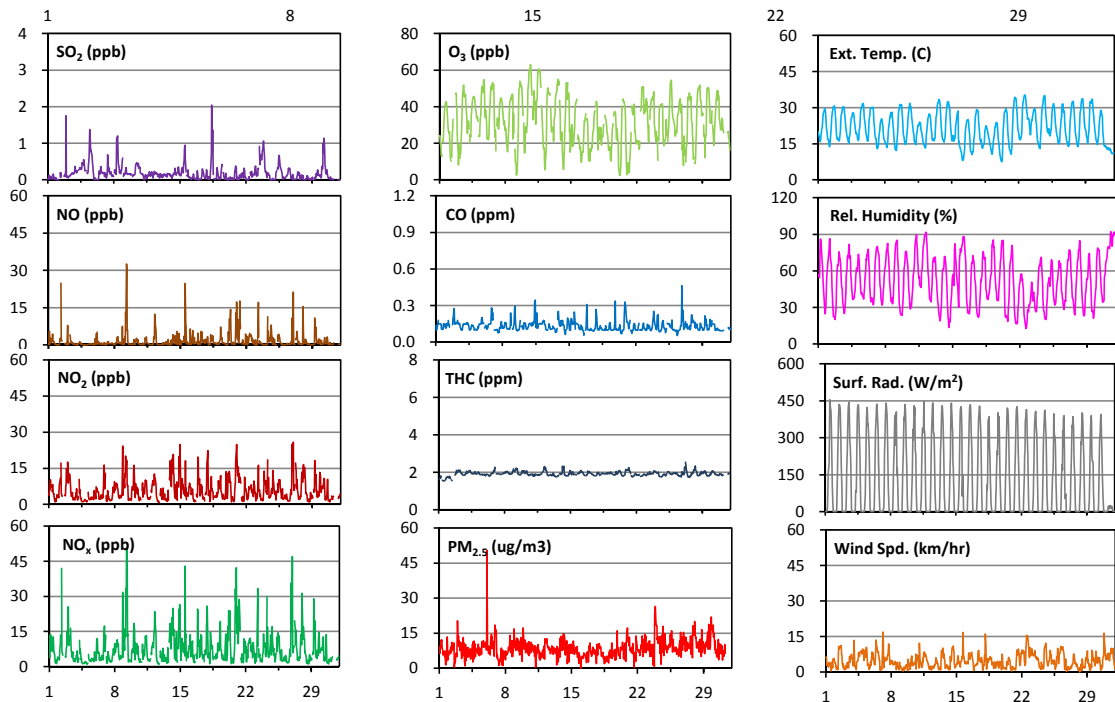



Palliser Airshed Society - August 2011 Summary Report

Continuous Sampling Results - Crescent Heights Station


Pollutants	Month Records	24-Hour Records						1-Hour Records					
		Name	Conc Unit	Avg. Conc.	Uptime	Maximum		AAAQO Objective	Exceed No.	Maximum		AAAQO Objective	Exceed No.
						Conc	Time			Conc	Time		
SO ₂	ppb	0.2	100.0%	0.5	Aug-23	48	0	2	Aug-18 9:00	172	0		
NO	ppb	2	100.0%	5	Aug-9	-	-	33	Aug-09 7:00	-	-		
NO ₂	ppb	6	100.0%	11	Aug-14	-	0	26	Aug-27 0:00	159	0		
NO _x	ppb	7	100.0%	13	Aug-20	-	-	51	Aug-09 7:00	-	-		
O ₃	ppb	32	100.0%	47	Aug-11	-	0	63	Aug-10 17:00	82	0		
CO	ppm	0.1	100.0%	0.2	Aug-11	-	0	0.5	Aug-26 21:00	13	0		
THC	ppm	1.9	100.0%	2	Aug-9	-	-	2.6	Aug-27 6:00	-	-		
PM _{2.5}	µg/m ³	8.5	97.7%	12.7	Aug-29	30	-	50.5	Aug-06 2:00	-	-		

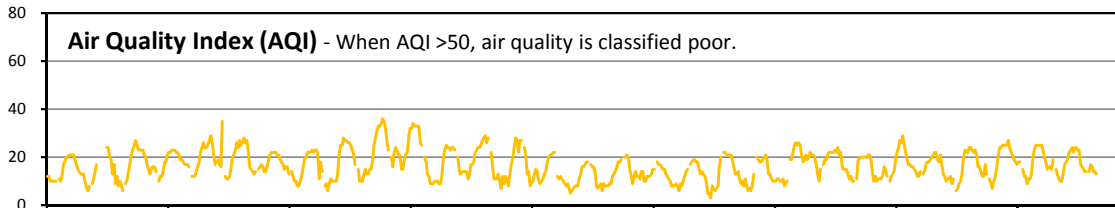

Instrument Uptime (%)

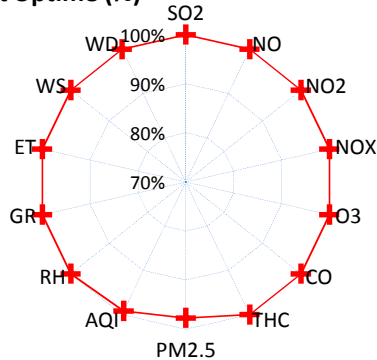


Wind Rose (km/hr)

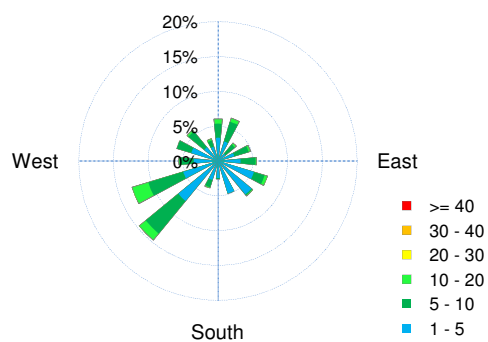


Palliser Airshed Society - August 2011 Summary Report

Passive Sampling Results

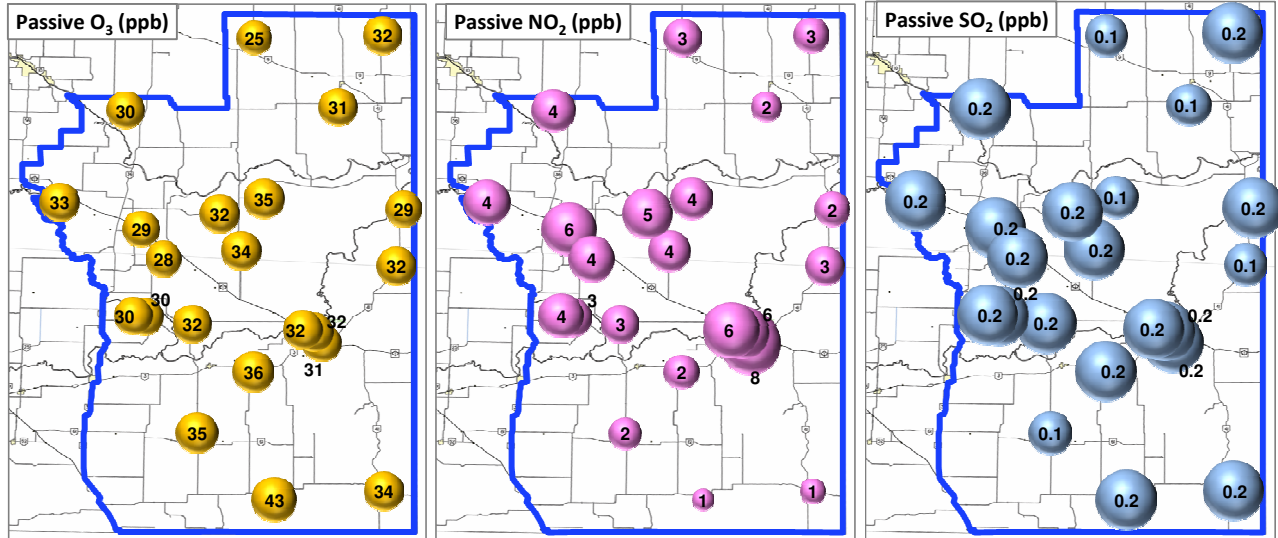


Rover Station Sampling Results - Hays Station


Pollutants	Month Records	24-Hour Records				1-Hour Records							
		Name	Conc Unit	Avg. Conc.	Uptime	Maximum		AAAQO Objective	Exceed No.	Maximum		AAAQO Objective	Exceed No.
						Conc	Time			Conc	Time		
SO ₂	ppb	0.1	100.0%	0.3	Aug-21	48	0	1.3	Aug-30 23:00	172	0		
NO	ppb	1	98.1%	2	Aug-20	-	-	13	Aug-04 19:00	-	-		
NO ₂	ppb	2	98.1%	4	Aug-28	-	0	16	Aug-28 21:00	159	0		
NO _x	ppb	3	98.1%	5	Aug-28	-	-	25	Aug-04 19:00	-	-		
O ₃	ppb	31	100.0%	38	Aug-11	-	0	60	Aug-10 17:00	82	0		
H ₂ S	ppb	0	100.0%	1	Aug-12	3	0	4	Aug-12 6:00	10	0		

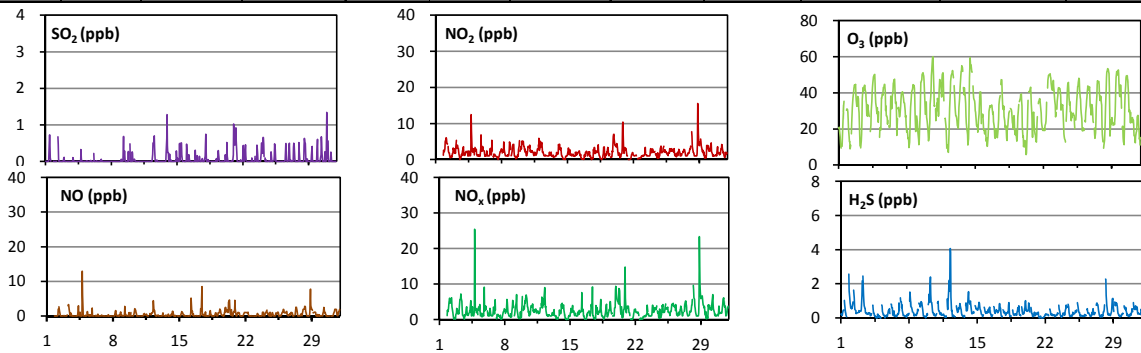

Instrument Uptime (%)



Wind Rose (km/hr)

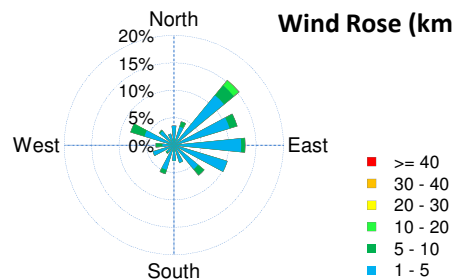

Monthly Update

- * The measured ambient concentrations of all parameters are within the AAAQO for the month of August 2011.
- * Crescent Heights station passes internal station audit on August 31, 2011.
- * The wind sensor of Hays station was malfunctioning from August 18 due to loose screws. It has been fixed on September 1.
- * Instrument maintenance: The PM2.5 monitor (Crescent Heights) and NO_x monitor (Portable Hays) were malfunctioning for part of the time in July. These two monitors were repaired on August 1, and were >90% operational for the month of August.